

Instrument: **HOCT-1F and HFC-1**

Subject: **Installation guide for Vuno Fundus AI software**

Status: **Informational**

Document Number: **TCM(R0)-210525-001**

Date: **25 APL 2021**

Pages: **10**



Table of Contents

1. How to install the VUNO Med-Fundus-AI
2. How to upgrade the HOCT & HFC software version
3. How to register a software license
4. How to use the AI function

1. How to install the VUNO Med-Fundus-AI

Vuno SW download link: <https://drive.google.com/file/d/1pD-bdqb1dtT3HNB24jw5vAhoslynKOud/view>



- 1) Run the Setup file.
- 2) Make sure opt-in a check box and press the Next button.
- 3) Press the Install button.

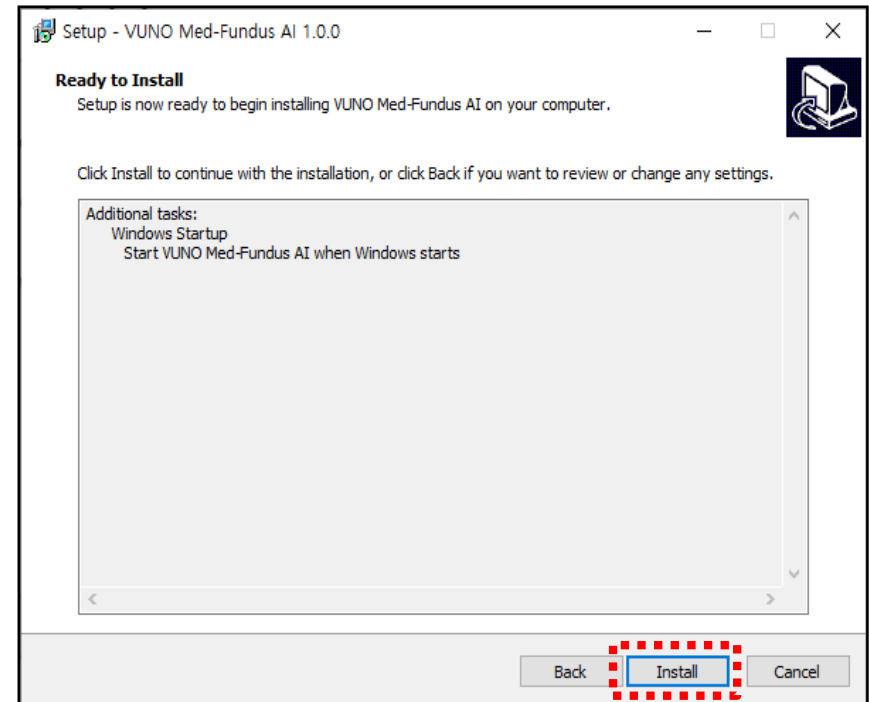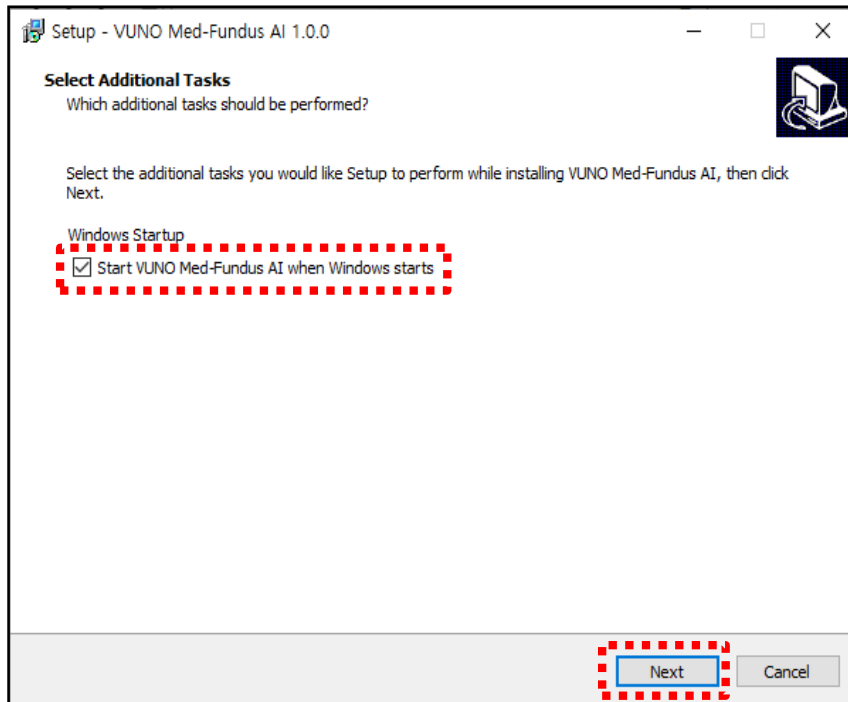

1. How to install the VUNO Med-Fundus-AI

4) When the progress bar is full, it goes to the completion screen.

5) Click the Finish button to close the Setup Wizard.

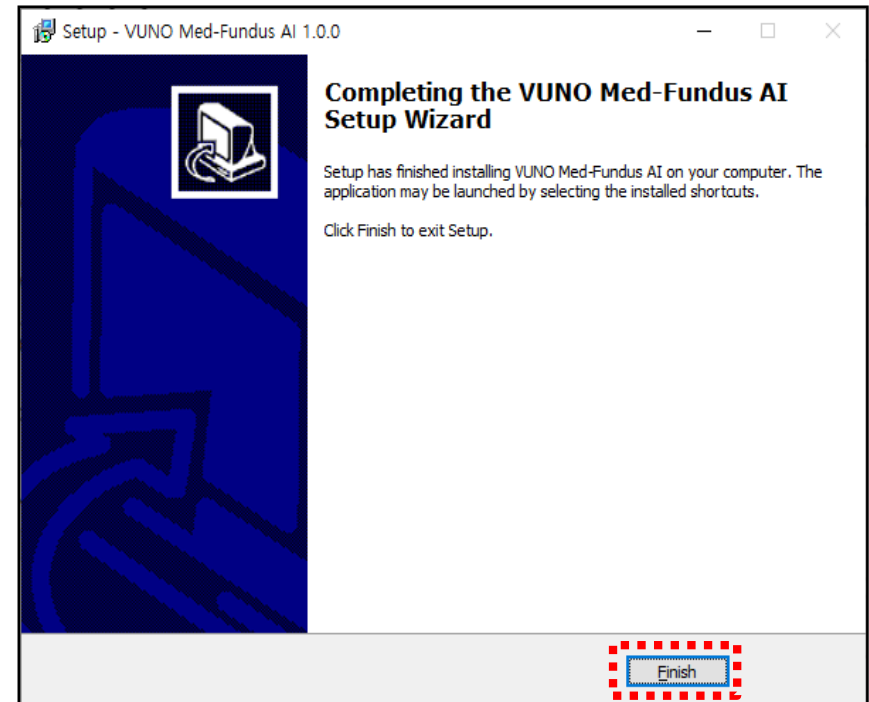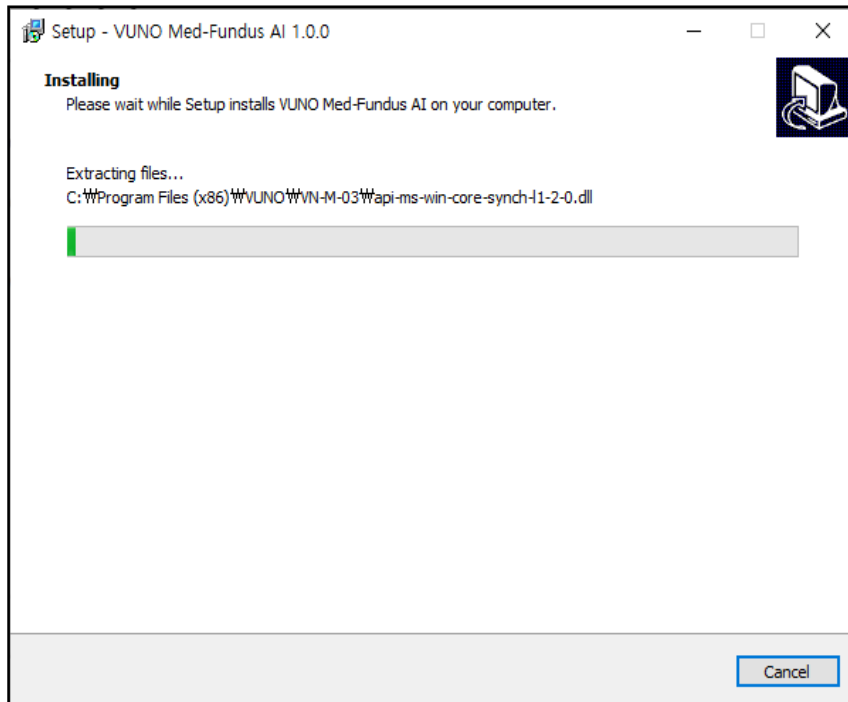



2. How to upgrade the HOCT & HFC software version

HOCT-1F SW download link:

https://drive.google.com/file/d/1ma8RnjMO4FyuxnloJBmCl53_sNfDu8yk/view?usp=drive_link

1) Run the Setup file.



2) Press the Next and I Agree button.

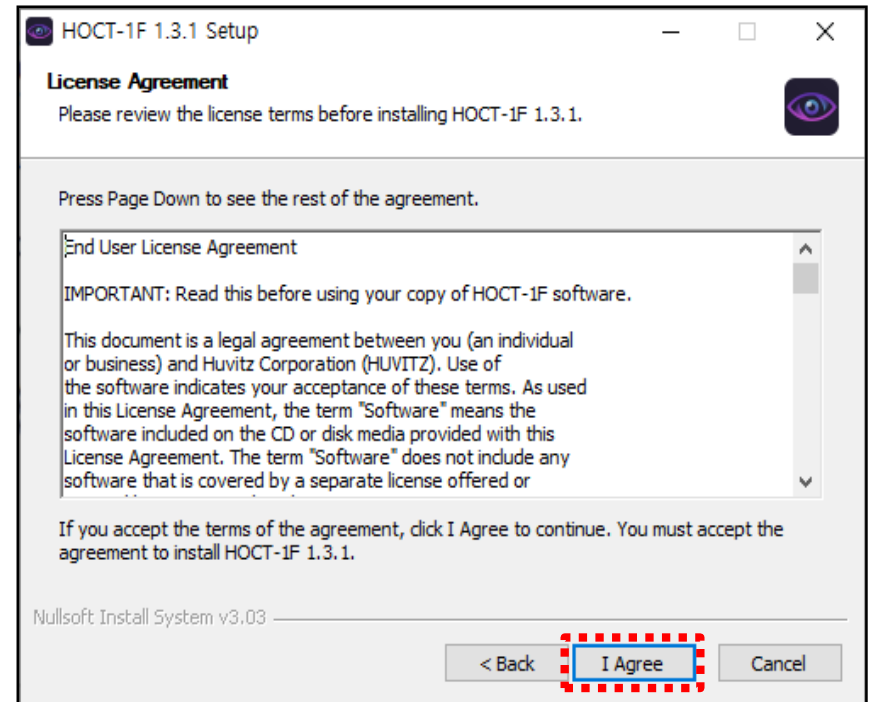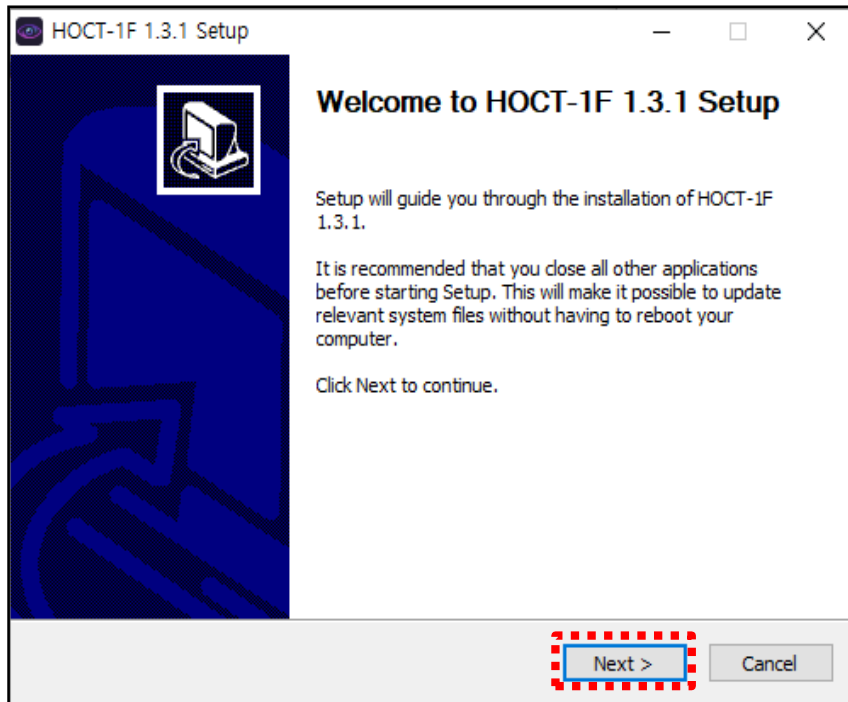

2. How to upgrade the HOCT & HFC software version

3) When the progress bar is full, it goes to the completion screen.

4) Make sure opt-in a check box and click the Finish button to close the Setup Wizard.

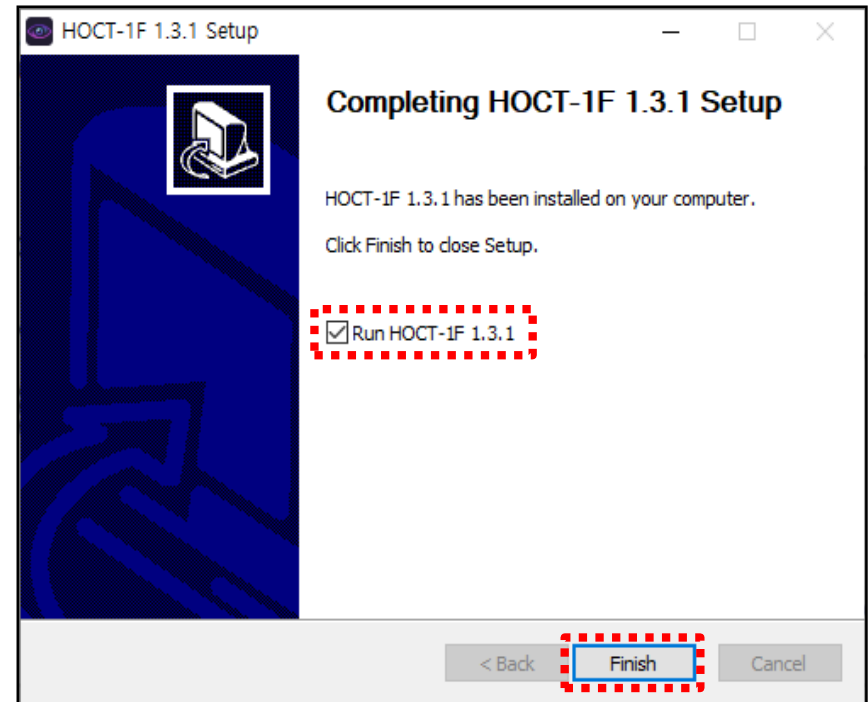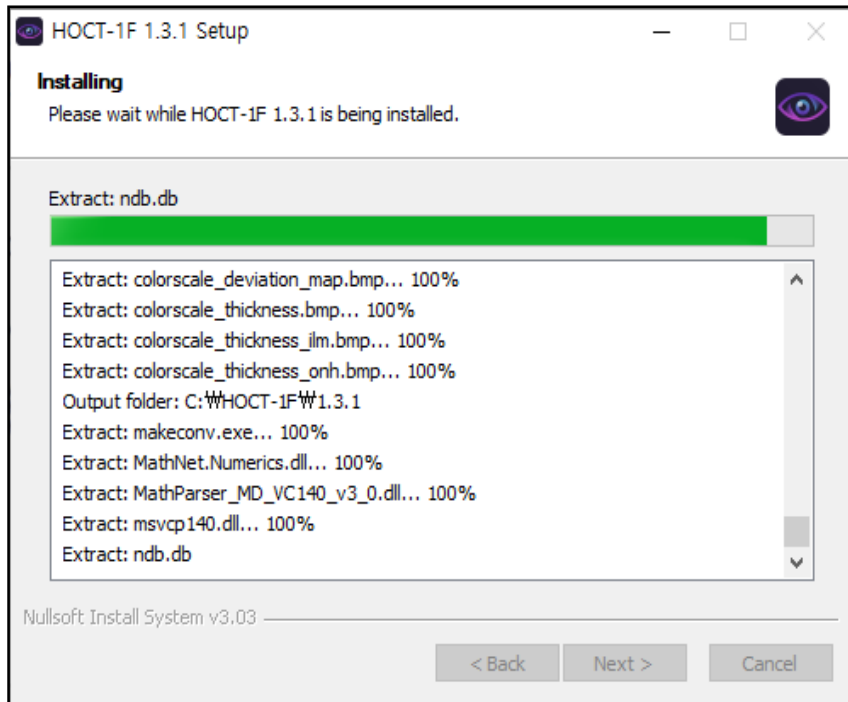

3. How to register a software license

- How to get unique key (UUID)

1) Install UUID Agent SW:


https://drive.google.com/file/d/1kXftxBh7pxUEWDxkIP2Gpk28s2ziDsSk/view?usp=drive_link

2) Check box of 'include disk serial'

3) Click 'get'



4) Click 'copy text'

5) Send unique key (UUID) to Huvitz sales team email, we will issue the License key.

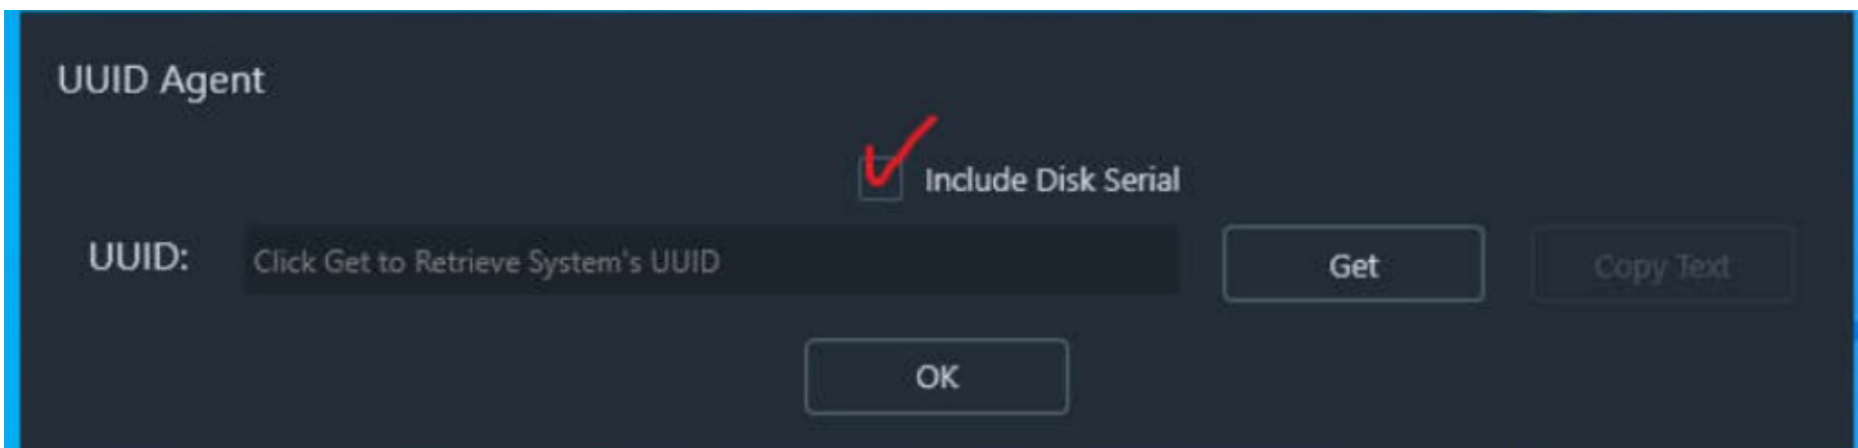

3. How to register a software license

- 1) Press the Setup icon on the main screen.
- 2) Go to the Info. tab and select VUNO AI.

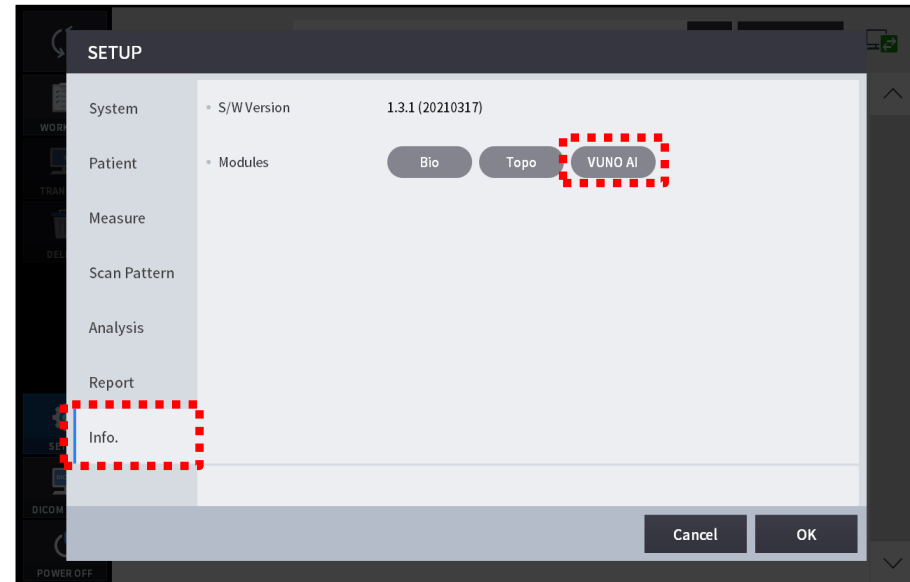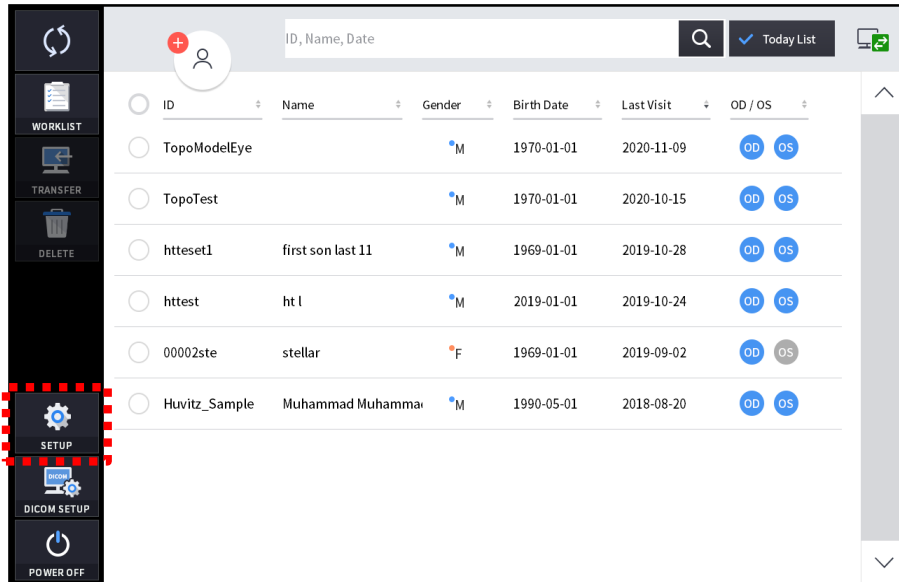

4. How to use the AI function

- 1) Select a patient to be analyzed from the main screen.
- 2) Select Fundus image and enter the analysis screen.

ID	Name	Gender	Birth Date	Last Visit	OD / OS
SM-30549814	CNV /AMD -Kim	F	1953-01-01	2018-11-20	OD OS
SG-24329973	Glaucoma -Kwack	M	1959-01-01	2018-10-23	OD OS
SH-31478181	High Myopia -Choi	F	1952-01-01	2018-09-28	OD OS
SM-11525696	ERM -Lee	F	1953-01-01	2018-09-14	OD OS
KD-130194286	PDR -Park	F	1958-06-14	2018-08-30	OD OS
KD-180147806	CNV -Park	F	1979-08-05	2018-08-21	OD OS
KD-970128233	CME -Jeon	M	1996-11-28	2018-08-21	OD OS
KD-120053876	RVO -Kim	M	1958-06-04	2018-08-14	OD OS
KD-170232956	PDR -Back	F	1959-04-14	2018-08-09	OD OS

Patient ID: SM-30549814
 Name: CNV /AMD -Kim
 Gender: F
 Birth Date: 1953-01-01
 Ethnicity: Asian
 Refraction: OD 0.00 OS 0.00
 Operator: _____ Physician: _____

OD		OS	
Anterior Radial 18-11-20 12:26:54	Disc 3D (H) 18-11-20 12:25:48	Fundus 18-11-20 12:14:35	
Macular Wide 18-11-20 12:14:31			

4. How to use the AI function

3) Click the VUNO icon to turn the AI function on and off.

4) If AI function is activated, the AI analysis screen is shown like the right picture.

